
Chroma Viewer

CHROMA examination review and database connectivity


EVOptica




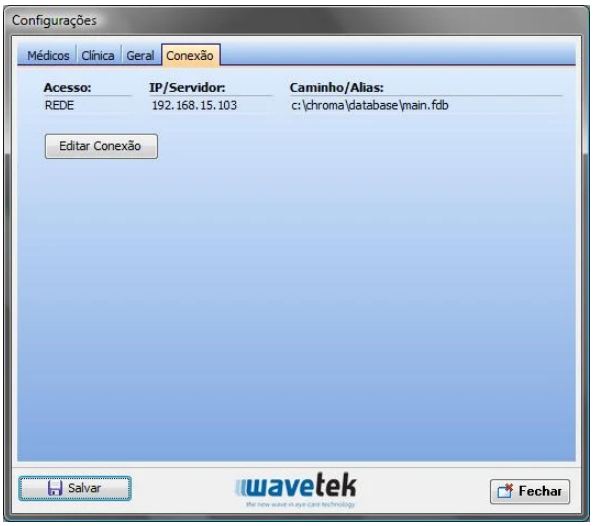

CHROMA Viewer - Examination Review

CHROMA Viewer accesses CHROMA system data locally or remotely from a computer that does not need to be physically connected to the CHROMA instrument. The required Viewer software and access to the CHROMA database are still needed; remote access uses the configured network/database connection.

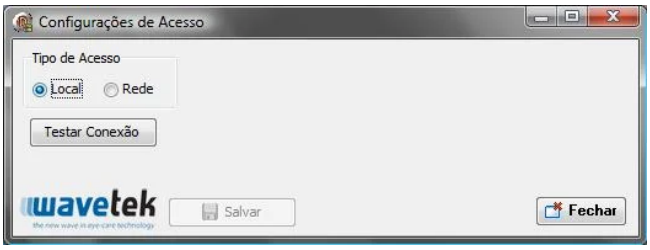

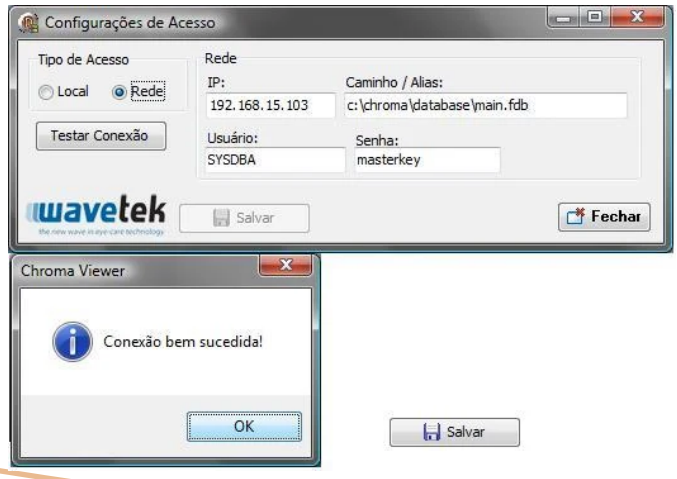

Software Screens and Connection Setup

Home screen - Click Settings > Display (Configurações > Exibir).

Settings screen - Access the Physicians (Médicos), Clinic (Clínica), General (Geral) and Connection (Conexão) tabs.

Click Edit Connection (Editar Conexão) to open Access Settings. The physician can choose local or network access and decide whether to save a successfully tested configuration.

For Network (Rede) access, enter the IP address, database path or alias, username and password.

Save option - The software permits a connection configuration to be saved only after a successful connection test.

Failed connection test - If the database is not found, the software displays a warning and prevents saving the unsuccessful configuration. This avoids replacing the saved connection with settings that did not pass the test.

EVOptica | evoptica.com | contact@evoptica.com

+1-315-210-8976 (call/text) | 221 S Main St, Fairport, NY 14450, USA